

Error induced by the estimation of the corneal power and the effective lens position with a rotationally asymmetric refractive multifocal intraocular lens

David P. Piñero^{1,2,3}, Vicente J. Camps¹, María L. Ramón², Verónica Mateo¹, Rafael J. Pérez-Cambrodí^{2,3}

¹Grupo de Óptica y Percepción Visual (GOPV). Department of Optics, Pharmacology and Anatomy, University of Alicante, San Vicente del Raspeig, Alicante 03690, Spain

²Department of Ophthalmology (Oftalmar), Vithas Medimar International Hospital, Alicante 03016, Spain

³Foundation for the Visual Quality (FUNCAVIS: Fundación para la Calidad Visual), Alicante 03016, Spain

Correspondence to: David P. Piñero. Department of Ophthalmology (OFTALMAR), 1st floor, Medimar International Hospital, C/Padre Arrupe 20, Alicante 03016, Spain. dpinero@oftalmar.es

Received: 2014-09-02

Accepted: 2014-12-01

Abstract

• **AIM :** To evaluate the prediction error in intraocular lens (IOL) power calculation for a rotationally asymmetric refractive multifocal IOL and the impact on this error of the optimization of the keratometric estimation of the corneal power and the prediction of the effective lens position (ELP).

• **METHODS:** Retrospective study including a total of 25 eyes of 13 patients (age, 50 to 83y) with previous cataract surgery with implantation of the Lentis Mplus LS-312 IOL (Oculentis GmbH, Germany). In all cases, an adjusted IOL power (P_{IOLadj}) was calculated based on Gaussian optics using a variable keratometric index value (n_{kadj}) for the estimation of the corneal power (P_{kadj}) and on a new value for ELP (ELP_{adj}) obtained by multiple regression analysis. This P_{IOLadj} was compared with the IOL power implanted ($P_{IOLReal}$) and the value proposed by three conventional formulas (Haigis, Hoffer Q and Holladay I).

• **RESULTS:** $P_{IOLReal}$ was not significantly different than P_{IOLadj} and Holladay IOL power ($P > 0.05$). In the Bland and Altman analysis, P_{IOLadj} showed lower mean difference (-0.07 D) and limits of agreement (of 1.47 and -1.61 D) when compared to $P_{IOLReal}$ than the IOL power value obtained with the Holladay formula. Furthermore, ELP_{adj} was significantly lower than ELP calculated with other conventional formulas ($P < 0.01$) and was found to be dependent on axial length, anterior chamber depth and P_{kadj} .

• **CONCLUSION:** Refractive outcomes after cataract surgery with implantation of the multifocal IOL Lentis Mplus LS -312 can be optimized by minimizing the

keratometric error and by estimating ELP using a mathematical expression dependent on anatomical factors.

• **KEYWORDS:** Mplus; multifocal intraocular lens; keratometry; effective lens position; intraocular lens power

DOI:10.3980/j.issn.2222-3959.2015.03.12

Piñero DP, Camps VJ, Ramón ML, Mateo V, Pérez-Cambrodí RJ. Error induced by the estimation of the corneal power and the effective lens position with a rotationally asymmetric refractive multifocal intraocular lens. *Int J Ophthalmol* 2015;8(3):501-507

INTRODUCTION

Several studies^[1-8] have confirmed the ability of multifocal intraocular lenses (IOLs) of providing a good near and distance functional vision without the use of corrective lenses after cataract surgery. One modality of IOL multifocality is the use of a rotationally asymmetric refractive profile containing an aspheric distance-vision zone combined with a sector-shaped near-vision zone in the inferior area of the IOL. This concept of multifocality is the basis of the multifocal IOL Lentis Mplus LS-312 (Oculentis GmbH). Studies on this IOL have shown good near and distance visual outcomes, combined with postoperative contrast sensitivity within physiological ranges and positive impact on patient's quality of life^[1,2,9-15]. Even some studies have reported good levels of intermediate visual acuity with this type of IOL^[1,2].

Despite the good visual outcomes reported with this IOL^[1,2,9-15], some studies have shown some level of variability in the refractive correction achieved^[1,2,9,13-15]. Alió *et al*^[15] found in a prospective comparative study evaluating a group of 21 eyes implanted with the Mplus IOL a mean 3mo postoperative sphere of -0.34 ± 0.93 D, ranging from -3.00 to +1.25 D. In another sample of 9366 eyes implanted with this type of IOL, Venter *et al*^[9] found that 91.8% of eyes had a postoperative spherical equivalent (SE) within ± 1.00 D. In the same line, Muñoz *et al*^[13] found that 6 eyes (9.4%) from a sample of 64 eyes had a postoperative myopic SE of more than 0.50 D (mean residual SE: -0.75 ± 0.15 D). McAlinden and Moore^[14] reported in another series of cases a percentage of 86.4% of eyes with an SE within ± 0.50 D. Several factors may be in relation to this variable level of predictability, such as some

inaccuracies in IOL power calculation due to the use of not fully optimized formulae for this specific type of IOL.

The aim of the current study was to evaluate the predictability of the refractive correction achieved with this refractive multifocal IOL and to develop an optimization of the predictability error by minimizing the error associated to the keratometric estimation of the corneal power and by developing a predictive formula of the effective lens position for this specific type of IOL.

SUBJECTS AND METHODS

Subjects This retrospective study included a total of 25 eyes of 13 patients. All eyes underwent cataract surgery with implantation of the rotationally asymmetric multifocal IOL Lentic Mplus LS-312 (Oculentis GmbH). Inclusion criteria for this study were patients with visually significant cataract or presbyopic/pre-presbyopic patients suitable for refractive lens exchange and demanding complete spectacle independence. Exclusion criteria were patients with active ocular diseases, illiteracy and topographic astigmatisms higher than 1.5 D. All volunteers were adequately informed about the surgery and signed a consent form. The study adhered to the tenets of the Declaration of Helsinki and was approved by the Local Ethical Committee.

Methods

Intraocular lens The Lentic Mplus LS-312 (Oculentis GmbH, Germany) is a rotationally asymmetric multifocal IOL that contains an aspheric distance-vision zone combined with a 3.00 D posterior sector-shaped near-vision zone to allow good transition between the zones. It has biconvex design with a 6.0 mm optic, a 12.0 mm overall length, and a C-loop haptic design with 0-degree angulation. The IOL is made of an acrylic copolymer comprising acrylates with a hydrophobic surface and ultraviolet-filtering components.

Surgical technique All surgeries were performed by the same experienced surgeon (Ramón ML) using a standard technique of phacoemulsification. In all cases, topical anesthesia was administered and pupillary dilation was induced with a combination of tropicamide and phenylephrine 10% every 15min half an hour previous to the procedure. Iodine solution 5% was instilled on the eye 10min before the operation. A 2.75-mm clear incision was made with a diamond knife on the steepest meridian to minimize post-surgical astigmatism. A paracentesis was made 60°-90° clockwise from the main incision and the anterior chamber was filled with viscoelastic material. After the crystalline lens removal, the IOLs were implanted through the incision into the capsular bag using a specific injector developed by the manufacturer for such purpose. Finally, the surgeon proceeded to retrieve the viscoelastic material using the irrigation-aspiration system. A combination of topical steroid and antibiotic (Tobradex, Alcon, Fort Worth, TX, USA) as

well as a non-steroidal anti-inflammatory drops (Dicloabak, Laboratorios Thea, Barcelona, Spain) were prescribed to be applied four times daily for a week after the surgery and three times daily the second postoperative week. In addition, non-steroidal anti-inflammatory drops were also prescribed to be applied three times daily during 2 additional weeks after surgery.

Calculation of an adjusted intraocular lens power

Almost all theoretical formulas for IOL power (P_{IOL}) calculation are based on the use of a simplified eye model, with thin cornea and lens models [16]. According to such approach, P_{IOL} can be easily calculated using the Gauss equations in paraxial optics:[17]

$$P_{IOL} = \left(\frac{n_{hv}}{AL - ELP} \right) - \left(\frac{n_{ha}}{\left(\frac{n_{ha}}{R_{des} + P_c} - ELP \right)} \right) \tag{1}$$

where, P_c is the total corneal power, ELP the effective lens plane, AL the axial length, n_{ha} the aqueous humour refractive index, n_{hv} the vitreous humour refractive index, and R_{des} the postoperative desired refraction calculated at corneal vertex.

Our research group proposed the use of a variable keratometric index (n_{kadj}) depending on the radius of the anterior corneal surface (r_{ic}) expressed in millimetres for minimizing the error associated to the keratometric approach for corneal power calculation [18]. Specifically, the following expression was defined according to the Gullstrand eye model:

$$n_{kadj} = -0.0064286r_{ic} + 1.37688 \tag{2}$$

Using these algorithm, a new keratometric corneal power, named adjusted keratometric corneal power (P_{kadj}), can be calculated using the classical keratometric corneal power formula [18]. In the current study, the adjusted IOL power (P_{IOLadj}) was calculated, which was defined as the IOL power calculated from the equation 1 using the n_{kadj} value for the estimation of the corneal power (P_{kadj}), and the n_{ha} and n_{hv} values corresponding to the Gullstrand eye model (1.336 for both indexes). In this IOL power calculation, the postoperative SE at corneal vertex was considered as the desired refraction ($R_{des}=SE_{post}$). The $PIOL_{adj}$ calculation was performed by estimating the ELP using two different approaches: ELP calculation following the SRK/T formula guidelines (named $P_{IOLadjSRK/T}$) [19] and ELP calculation using a mathematical expression obtained by multiple regression analysis (named P_{IOLadj}), following a procedure described in the next section. These values of IOL power (P_{IOLadj}) were compared with the real power of the IOL implanted ($P_{IOLReal}$).

An P_{IOL} calculation was also performed using three conventional formulae (Haigis [20], Hoffer Q [21] and Holladay

I^[22]) considering the ELP defined for each formula and $R_{des}=SE_{post}$. All these values of P_{IOL} were also compared to P_{IOLadj} . The calculation with the conventional IOL power formulas was performed by implementing them in an Excel software sheet version 14.0.0 for Mac.

Estimation of adjusted effective lens position

Considering the equation 1, $P_{IOLreal}$, P_{kadj} and $R_{des}=SE_{post}$, an estimation of ELP was obtained in each case. By means of multiple regression analysis, a mathematic expression was obtained for predicting the ELP in each specific case. This ELP was named as adjusted effective lens position (ELP_{adj}).

Preoperative and postoperative examinations

Preoperatively, all patients had a full ophthalmologic examination including the evaluation of the refractive status, distance and near visual acuities, slit lamp examination, optical biometry (IOL-Master, Zeiss), applanation tonometry and funduscopy. Distance (4 m) and near (40 cm) visual acuities were evaluated with ETDRS charts. Postoperatively, patients were evaluated at 1d, 1wk, 1mo and 3mo after surgery. In all visits, visual acuity, refraction and the integrity of the anterior segment were evaluated. Funduscopy was also performed in the postoperative revision at 3mo.

Statistical Analysis The statistical analysis was performed using the SPSS statistics software package version 21.0.0.0 for Mac (IBM, Armonk, NY, USA). Normality of data samples was evaluated by means of the Kolmogorov-Smirnov test. When parametric analysis was possible, the Student *t* test for paired data was used for comparing the different approaches for P_{IOL} calculation. When parametric analysis was not possible, the Wilcoxon rank sum test was applied to assess the significance of such comparisons. Differences were considered to be statistically significant when the associated *P*-value was of less than 0.05. Regarding the interchangeability between pairs of methods for obtaining P_{IOL} , the Bland-Altman analysis was used^[23].

A multiple regression analysis was performed by using the backward elimination method for obtaining a mathematical expression allowing the prediction of ELP_{adj} from different preoperative anatomical and clinical parameters. Model assumptions were evaluated by analysing residuals, the normality of non-standardized residuals (homoscedasticity), and the Cook distance to detect influential points or outliers. In addition, the lack of correlation between errors and multicollinearity was assessed using the Durbin-Watson test, the calculation of the colinearity tolerance, and the variance inflation factor.

RESULTS

This study evaluated 25 eyes of 13 patients [6 men (46.2%) and 7 women (53.8%)], with a mean age of 65.6y±7.6 SD (range, 50 to 83y). The sample comprised 12 (48%) and 13 (52%) right and left eyes, respectively. Table 1 summarizes some preoperative visual, refractive and anatomical data of

Table 1 Summary of several parameters involved in the study: mean preoperative anatomical and corneal power (calculated with the conventional keratometric index 1.3375, the Haigis approach^[20] and the approach developed by our research group^[18]) parameters, mean preoperative and postoperative SE, mean n_{kadj} (calculated with our approach^[18]), and mean ELP and IOL power calculated with different formulas

Parameters	$\bar{x} \pm s$	Range
SE _{pre} (D)	-1.27± 2.87	-7.50 to 3.00
SE _{post} (D)	-0.11±0.56	-1.83 to 0.76
r _{1c} ^[24]	7.61 ± 0.25	7.19 to 8.01
ACD ^[24]	3.31 ± 0.28	2.61 to 3.79
AL ^[24]	23.52 ± 1.04	22.02 to 27.36
ELP _{SRK/T} ^[24]	5.12 ± 0.45	4.60 to 6.83
ELP _{adj} ^[24]	4.31 ± 0.50	3.39 to 5.34
ELP _{Haigis} ^[24]	5.01 ± 0.16	4.77 to 5.46
ELP _{HofferQ} ^[24]	5.00 ± 0.27	4.63 to 6.01
ELP _{Holladay} ^[24]	4.59 ± 0.27	3.89 to 5.07
n_{kadj}	1.328 ± 0.002	1.325 to 1.331
$P_{k(1.3375)}$ (D)	44.37 ± 1.44	42.14 to 46.95
$P_{cHaigis}$ (D)	43.57 ± 1.41	41.39 to 46.11
P_{kadj} (D)	43.11 ± 1.61	40.62 to 45.99
$P_{IOLReal}$ (D)	19.78 ± 2.32	12.50 to 23.50
$P_{IOLadjSRK/T}$ (D)	21.18 ± 2.74	12.51 to 25.46
P_{IOLadj} (D)	19.71 ± 2.55	11.02 to 23.53
$P_{IOLHaigis}$ (D)	20.40 ± 3.15	10.16 to 24.99
$P_{IOLHofferQ}$ (D)	19.30 ± 3.04	9.50 to 23.90
$P_{IOLHolladay}$ (D)	19.57 ± 2.99	9.40 to 23.90

SE_{pre}: Preoperative spherical equivalent; SE_{post}: Postoperative spherical equivalent; r_{1c}: Radius of curvature of the anterior corneal surface; ACD: Anterior chamber depth; AL: Axial length; ELP_{SRK/T}: Effective lens position for the SRK/T formula; ELP_{adj}: Effective lens position for the adjusted formula; ELP_{Haigis}: Effective lens position for the Haigis formula; ELP_{HofferQ}: Effective lens position for the Hoffer Q formula; ELP_{Holladay}: Effective lens position for the Holladay formula; n_{kadj} : Adjusted keratometric index; $P_{k(1.3375)}$: Corneal power obtained using IOL-Master or keratometric power; $P_{cHaigis}$: Corneal power obtained for the Haigis formula; P_{kadj} : Corneal power obtained using the adjusted keratometric index; $P_{IOLReal}$: Power of the intraocular lens implanted which was calculated using the SRK/T formula; $P_{IOLadjSRK/T}$: Power of the intraocular lens obtained using adjusted formula and ELP calculated with the SRK/T formula; P_{IOLadj} : Intraocular lens power obtained using the adjusted formula and ELP_{adj}; $P_{IOLHaigis}$: Intraocular lens power obtained using the Haigis formula; $P_{IOLHofferQ}$: Intraocular lens power obtained using the Hoffer Q formula; $P_{IOLHolladay}$: Intraocular lens power obtained using the Holladay formula.

the eyes evaluated as well as all the estimation performed for ELP and IOL power. According to axial length (AL), anterior chamber depth (ACD) and corneal power, and using the SRK-T formula, the mean power of the IOL implanted was 19.78 D±2.32 SD (range, 12.50 to 23.50 D).

Agreement of $P_{IOLReal}$ and $P_{IOLadjSRK/T}$ Statistically significant differences were found between $P_{IOLadjSRK/T}$ and $P_{IOLReal}$, considering that ELP was calculated following the SRK/T formula guidelines and considering $R_{des}=SE_{post}$ (*P* < 0.01, Wilcoxon test). A very strong and statistically significant correlation was found between P_{IOLadj} and $P_{IOLReal}$ (*r* = 0.86, *P* < 0.01, Figure 1). According to the Bland and Altman analysis of interchangeability, the $P_{IOLadjSRK/T}$ was higher than $P_{IOLReal}$ (mean difference: 1.41 D) and the limits of agreement

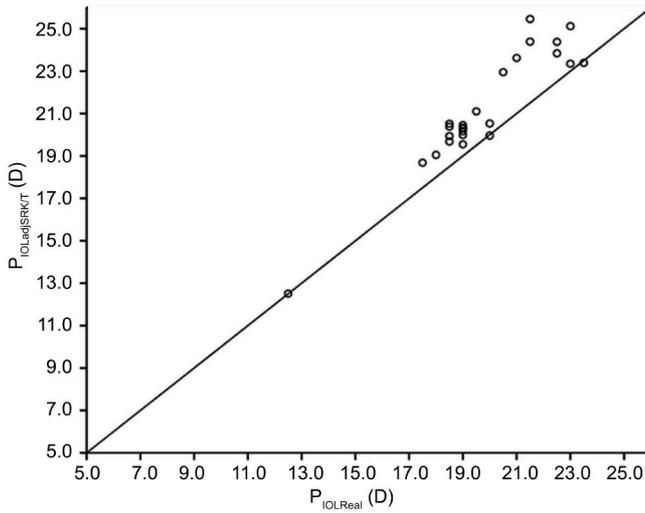


Figure 1 Relationship between the adjusted IOL power using the ELP estimated using the SRK/T formula guidelines ($P_{IOLadjSRK/T}$) and the real power of the IOL implanted ($P_{IOLReal}$).

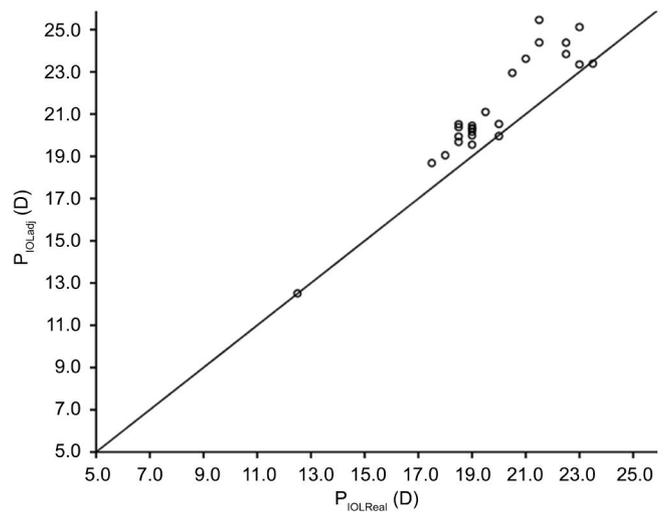


Figure 3 Relationship between the adjusted IOL power using the regression analysis adjusted ELP (P_{IOLadj}) and the real power of the IOL implanted ($P_{IOLReal}$).

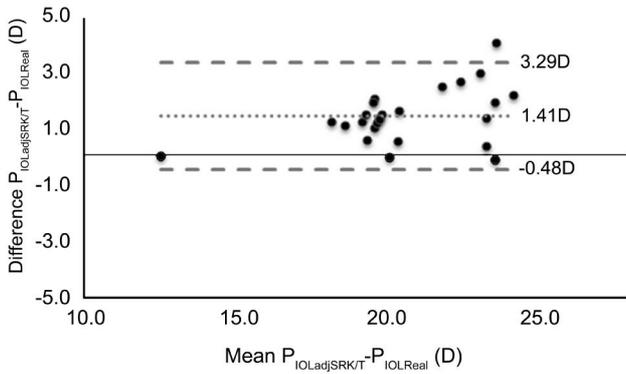


Figure 2 Bland–Altman plots for the comparison between the adjusted IOL power using the ELP estimated using the SRK/T formula guidelines ($P_{IOLadjSRK/T}$) and the real power of the IOL implanted ($P_{IOLReal}$). The dotted lines show the limits of agreement ($\pm 1.96SD$).

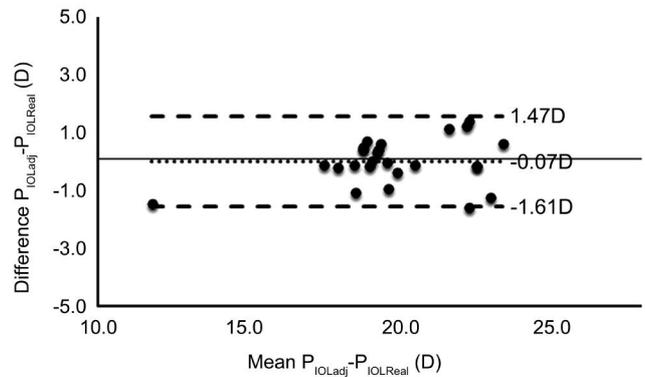


Figure 4 Bland–Altman plots for the comparison between the adjusted IOL power using the regression analysis adjusted ELP (P_{IOLadj}) and the real power of the IOL implanted ($P_{IOLReal}$). The dotted lines show the limits of agreement ($\pm 1.96SD$).

were clinically relevant (3.29 and -0.48 D). Figure 2 shows the Bland and Altman plot corresponding to this agreement analysis.

Estimation of ELP_{adj} The multiple regression analysis revealed that the ELP_{adj} was significantly correlated with AL, ACD and P_{kadj} ($P < 0.01$):

$$ELP_{adj} = -17.333 + 0.612 \times ACD + 0.360 \times AL + 0.268 \times P_{kadj} \quad (3)$$

The homoscedasticity of the model was confirmed by the normality of the non-standardized residuals distribution ($P = 0.20$) and the absence of influential points or outliers (mean Cook's distance: 0.155 ± 0.528). With this model, 56% of non-standardized residuals were 0.20 or lower and 76% were lower than 0.50. The poor correlation between residuals (Durbin-Watson test: 1.629) and the lack of multicollinearity (tolerance 0.805 to 0.560; variance inflation factors 1.785 to 1.243) was also confirmed.

A statistically significant difference was found between

ELP_{adj} and the rest of ELP values obtained following the guidelines proposed by each of the formulas used ($P < 0.01$, unpaired Wilcoxon test). ELP_{adj} was the lowest ELP value (Table 1) among all values of ELP calculated (4.31 ± 0.50 mm, range 3.39 to 5.34 mm).

Agreement between $P_{IOLReal}$ and P_{IOLadj} No statistically significant differences were found between P_{IOLadj} and $P_{IOLReal}$ when ELP_{adj} and $R_{des} = SE_{post}$ were considered for P_{IOLadj} calculation ($P = 0.65$, unpaired Student's t -test). A very strong and statistically significant correlation was found between P_{IOLadj} and $P_{IOLReal}$ ($r = 0.95$, $P < 0.01$) (Figure 3). According to the Bland and Altman [23] analysis, the mean difference between both P_{IOLadj} and $P_{IOLReal}$ was -0.07 D, with limits of agreement of 1.47 and -1.61 D. Figure 4 shows the Bland and Altman plot corresponding to this agreement analysis.

Agreement of P_{IOLadj} with other formulas Statistically significant differences were found between P_{IOLadj} and $P_{IOLHaigis}$, and between P_{IOLadj} and $P_{IOLHofferQ}$ ($P < 0.01$, Wilcoxon test), but not between P_{IOLadj} and $P_{IOLHolladay}$ ($P = 0.20$, Wilcoxon test).

Table 2 Bland and Altman analysis outcomes of the comparison between P_{IOLadj} and the IOL power obtained with other commonly used formulas

Comparison	$\Delta P_{IOL} \pm SD$ (D)	LoA (D)	P
$P_{IOLHaigis} - P_{IOLadj}$	0.68 ± 0.72	2.09 to -0.73	<0.01
$P_{IOLHofferQ} - P_{IOLadj}$	-0.43 ± 0.75	1.05 to -1.90	<0.01
$P_{IOLHolladay} - P_{IOLadj}$	-0.13 ± 0.67	1.01 to -1.28	0.20

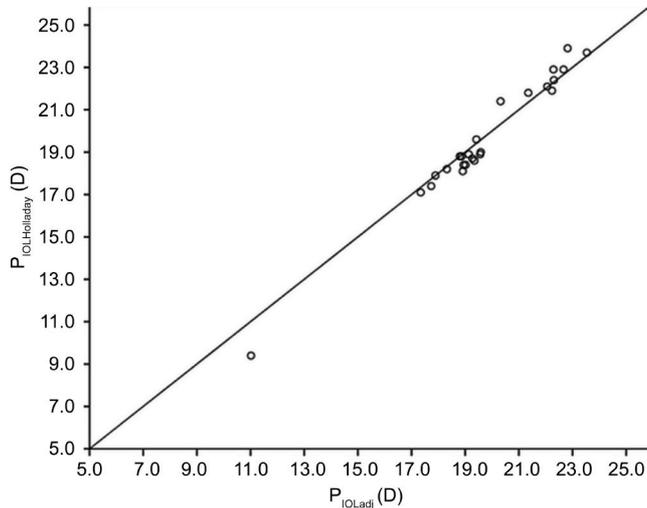


Figure 5 Relationship between the adjusted IOL power using the regression analysis adjusted ELP (P_{IOLadj}) and the IOL power when using the Holladay formula ($P_{IOLHolladay}$).

Table 2 shows the Bland and Altman analysis outcomes corresponding to all comparisons done. A very strong and statistically significant correlation was found between P_{IOLadj} and $P_{IOLHolladay}$ ($r=0.96$, $P<0.01$, Figure 5). According to the Bland and Altman [23] analysis, the mean difference between both P_{IOLadj} and $P_{IOLHolladay}$ was -0.13 D, with limits of agreement of 1.01 and -1.28 D. Figure 6 shows the Bland and Altman plot corresponding to this agreement analysis.

Agreement of $P_{IOLreal}$ with other formulas Statistically significant differences were found between $P_{IOLreal}$ and $P_{IOLHaigis}$, and between $P_{IOLreal}$ and $P_{IOLHofferQ}$ ($P<0.05$, Wilcoxon test), but not between $P_{IOLreal}$ and $P_{IOLHolladay}$ ($P=0.29$, Wilcoxon test). Table 3 shows the Bland and Altman analysis outcomes corresponding to all comparisons done. According to the Bland and Altman method, the mean difference between $P_{IOLHolladay}$ and $P_{IOLreal}$ was -0.21 D, with limits of agreement of 1.96 and -2.37 D (Figure 7).

DISCUSSION

The refractive results obtained after cataract surgery with implantation of a multifocal IOL based on the concept of refractive rotationally asymmetry, the Lentis LS-312 IOL, have been evaluated in the current series. A significant variability in the postoperative SE was observed in the analyzed sample, with a mean value of -0.11 ± 0.56 D. Specifically, the SE at 3mo after surgery ranged from -1.83 to +0.76 D, with a slight trend to some level of residual myopia, as in some previous series evaluating the results of the same

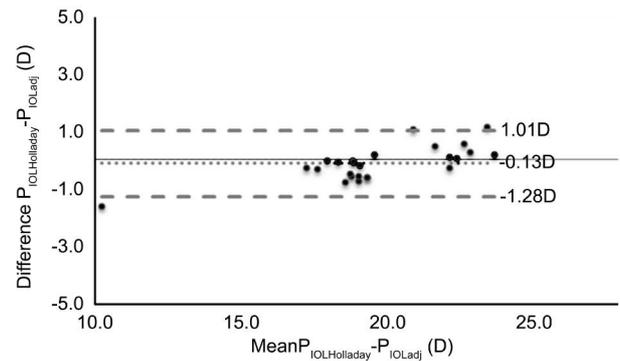


Figure 6 Bland–Altman plots for the comparison between the adjusted IOL power using the regression analysis adjusted ELP (P_{IOLadj}) and the IOL power when using the Holladay formula ($P_{IOLHolladay}$) The dotted lines show the limits of agreement (± 1.96 SD).

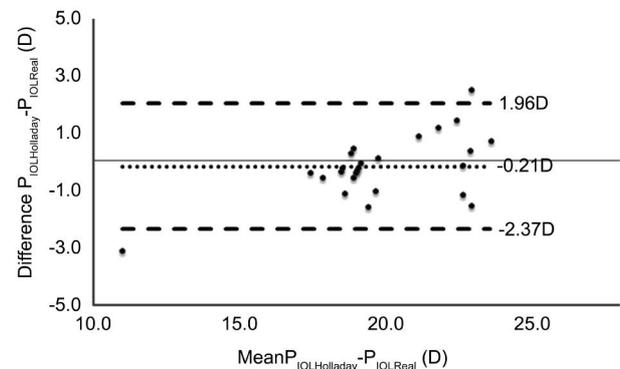


Figure 7 Bland–Altman plots for the comparison between the IOL power when using the Holladay formula ($P_{IOLHolladay}$) and the real power of the IOL implanted ($P_{IOLreal}$) The dotted lines show the limits of agreement (± 1.96 SD).

Table 3 Bland and Altman analysis outcomes of the comparison between $P_{IOLreal}$ and the IOL power obtained with other commonly used formulas

Comparison	$\Delta P_{IOL} \pm SD$ (D)	LoA (D)	P
$P_{IOLHaigis} - P_{IOLreal}$	0.62 ± 1.15	2.88 to -1.64	0.01
$P_{IOLHofferQ} - P_{IOLreal}$	-0.43 ± 1.13	1.73 to -2.69	0.03
$P_{IOLHolladay} - P_{IOLreal}$	-0.13 ± 1.10	1.96 to -2.37	0.29

type of multifocal IOL [21,15]. This confirms that an optimization in the algorithm of IOL power calculation is necessary in order to refine the refractive and visual outcomes with this premium multifocal IOL. The relative limitation of the predictability of the refractive correction in some cases implanted with the Mplus IOL may be attributable to the bias associated to the use of the keratometric approach for the calculation of the corneal power, errors in the determination of the axial length or inaccuracy in the estimation of the ELP for this specific IOL. However, the errors in the estimation of axial length with the technology used have been shown to be minimal and with a very limited impact on the refractive predictability [24]. Therefore, in the current study, the potential contribution of the corneal power and ELP factors to the limitation of the

refractive predictability with the multifocal IOL evaluated have been investigated.

First, the potential impact of the keratometric error was analysed by calculating the corneal power using an adjusted keratometric index aimed at minimizing the clinical error in the estimation of the corneal power^[17,18]. This adjusted corneal power was used to obtain an estimation of the IOL power considering the axial length and an ELP estimated following the algorithm established for the SRK-T formula^[19]. With this approach, statistically significant and clinically relevant differences were found between the adjusted calculation ($P_{IOLadjSRK/T}$) and the real power of the IOL implanted that was selected according to the SRK-T formula ($P_{IOLReal}$)^[19]. Therefore, the correction of this factor seems to have a minimal effect on the outcomes achievable with the multifocal IOL evaluated. Then, ELP was thought to be a critical factor for the presence of a relatively limited predictability with the IOL evaluated. For such purpose, an expression for estimating an optimized ELP according to some preoperative parameters was obtained by means of multiple linear regression. This new ELP estimation was named adjusted ELP (ELP_{adj}). The ELP_{adj} were compared to those ELP values obtained with other predicting algorithms of ELP^[19-21]. This analysis revealed that the ELP_{adj} was significantly lower compared to the values estimated with the Haigis, Hoffer Q and Holladay I formulas (ELP_{Haigis} , $ELP_{HofferQ}$ and $ELP_{Holladay}$ respectively)^[20,21]. In any case, differences between ELP_{adj} and $ELP_{Holladay}$ were found to be the lowest in magnitude and this may be the reason for the absence of statistically significant differences between P_{IOLadj} and $P_{IOLHolladay}$. In contrast, the difference was statistically significant and clinically relevant when our IOL power (P_{IOLadj}) was compared to Haigis or Hoffer Q formulas ($P_{IOLHaigis}$ and $P_{IOLHofferQ}$, respectively). One factor attributable to the lower value of ELP_{adj} compared to those ELP values obtained with conventional formulas is a more anterior position of the optic of the multifocal IOL evaluated due to the flexibility of the haptics. This more anterior position was better predicted with the Holladay formula and with our ELP_{adj} calculation algorithm (see equation 3). This may explain in part the trend toward myopia observed in our sample, in which the IOL power calculation was performed with the SRK-T formula that uses higher estimated values of ELP. Indeed, considering equation 1, a longer ELP would lead to the calculation of a higher value of IOL power that may potentially lead to the presence of postoperative myopia. Future studies should evaluate the real position of the IOL within the capsular bag by means of imaging techniques in order to confirm our hypotheses, as has been done for other types of IOLs^[25].

In our linear regression analysis, ELP_{adj} was found to be related to some factors, such as the AL, P_{kadj} and the ACD.

The anatomical factors were crucial determinants of the final position of the IOL evaluated within the eye. ELP_{adj} was higher in those eyes with longer AL and ACD, as happens in moderate to high myopic eyes. This finding was consistent with those reported by previous authors, reporting a linear dependence of the final position of the IOL on the AL^[26-28]. Considering that ELP_{adj} and $ELP_{Holladay}$ were not significantly different, this formula seems to be the most recommendable approach for IOL power calculation with the multifocal IOL evaluated. More studies with larger samples sizes should be performed to confirm all these outcomes.

Finally, it should be mentioned that when all IOL power formulas were compared with $P_{IOLReal}$, P_{IOLadj} and $P_{IOLHolladay}$ did not differ significantly with $P_{IOLReal}$. The Bland-Altman plots showed less clinically relevant level of agreement of $P_{IOLReal}$ with P_{IOLadj} than with $P_{IOLHolladay}$ (Figures 4, 7). Therefore, P_{IOLadj} was able to reproduce more accurately $P_{IOLReal}$ and therefore of the refractive outcome. This suggests that our approach may be a useful method for IOL power calculation with the multifocal IOL evaluated. This should be corroborated in future prospective studies.

There are several limitations in the current research, such as the limited sample size or the short follow-up. It should be considered that, although rare, changes in IOL position has been described more than 3mo after surgery, especially after Nd:YAG capsulotomy^[29]. This requires further analysis and investigation in future studies with the Mplus IOL. Another potential limitation is the determination of refraction with this multifocal IOL. Some difficulties have been described for obtaining an accurate refraction after implantation of different models of IOL, with a clear trend to overestimation of the sphere with positive sign^[30]. In any case, the manifest refraction was obtained using the same procedure described for refracting eyes with multifocal IOLs^[31] and without using the autorrefraction as the basis because it has been shown to fail in eyes implanted with the Mplus IOL^[32]. Finally, it should be mentioned that the Holladay II formula was not used in our comparison as it was not available in our clinic. Possibly, our approach may be more similar to the results of the Holladay II formula as both types of calculation use an optimized algorithm for the estimation of ELP, but this should be confirmed in future studies.

In conclusion, refractive outcomes after cataract surgery with implantation of refractive rotationally asymmetric IOL Lentis Mplus LS-312 may be optimized by minimizing the keratometric error using a variable keratometric index for corneal power estimation and by estimating ELP using a mathematical expression dependent on anatomical factors. Future studies should be performed to validate this model of IOL power calculation for the Lentis Mplus IOL with larger

sample of sizes including more extreme cases (long and short AL).

ACKNOWLEDGEMENTS

Conflicts of Interest: Piñero DP, None; Camps VJ, None; Ramón ML, None; Mateo V, None; Pérez-Cambrodí RJ, None.

REFERENCES

- 1 Ramón ML, Piñero DP, Pérez-Cambrodí RJ. Correlation of visual performance with quality of life and intraocular aberrometric profile in patients implanted with rotationally asymmetric multifocal IOLs. *J Refract Surg* 2012;28(2):93-99
- 2 Alió JL, Piñero DP, Plaza-Puche AB, Chan MJ. Visual outcomes and optical performance of a monofocal intraocular lens and a new-generation multifocal intraocular lens. *J Cataract Refract Surg* 2011;37(2):241-250
- 3 Alió JL, Plaza-Puche AB, Piñero DP, Amparo F, Jiménez R, Rodríguez-Prats JL, Javaloy J, Pongo V. Optical analysis, reading performance, and quality-of-life evaluation after implantation of a diffractive multifocal intraocular lens. *J Cataract Refract Surg* 2011;37(1):27-37
- 4 Alfonso JF, Fernández-Vega L, Puchades C, Montés-Micó R. Intermediate visual function with different multifocal intraocular lens models. *J Cataract Refract Surg* 2010;36(5):733-739
- 5 Kohnen T, Nuijts R, Levy P, Haefliger E, Alfonso JF. Visual function after bilateral implantation of apodized diffractive aspheric multifocal intraocular lenses with a +3.0 D addition. *J Cataract Refract Surg* 2009;35(12):2062-2069
- 6 Alfonso JF, Puchades C, Fernández-Vega L, Montés-Micó R, Valcárcel B, Ferrer-Blasco T. Visual acuity comparison of 2 models of bifocal aspheric intraocular lenses. *J Cataract Refract Surg* 2009;35(4):672-676
- 7 Alfonso JF, Fernández-Vega L, Señaris A, Montés-Micó R. Prospective study of the Acri.LISA bifocal intraocular lens. *J Cataract Refract Surg* 2007;33(11):1930-1935
- 8 Alfonso JF, Fernández-Vega L, Baamonde MB, Montés-Micó R. Prospective visual evaluation of apodized diffractive intraocular lenses. *J Cataract Refract Surg* 2007;33(7):1235-1243
- 9 Venter JA, Pelouskova M, Collins BM, Schallhorn SC, Hannan SJ. Visual outcomes and patient satisfaction in 9366 eyes using a refractive segmented multifocal intraocular lens. *J Cataract Refract Surg* 2013;39(10):1477-1484
- 10 van der Linden JW, van Velthoven M, van der Meulen I, Nieuwendaal C, Mourits M, Lapid-Gortzak R. Comparison of a new-generation sectorial addition multifocal intraocular lens and a diffractive apodized multifocal intraocular lens. *J Cataract Refract Surg* 2012;38(1):68-73
- 11 Alió JL, Plaza-Puche AB, Javaloy J, Ayala MJ, Moreno LJ, Piñero DP. Comparison of a new refractive multifocal intraocular lens with an inferior segmental near add and a diffractive multifocal intraocular lens. *Ophthalmology* 2012;119(3):555-563
- 12 Alfonso JF, Fernández-Vega L, Blázquez JJ, Montés-Micó R. Visual function comparison of 2 aspheric multifocal intraocular lenses. *J Cataract Refract Surg* 2012;38(2):242-248
- 13 Muñoz G, Albarrán-Diego C, Ferrer-Blasco T, Sakla HF, García-Lázaro S. Visual function after bilateral implantation of a new zonal refractive aspheric multifocal intraocular lens. *J Cataract Refract Surg* 2011;37(11):2043-2052
- 14 McAlinden C, Moore JE. Multifocal intraocular lens with a surface-embedded near section: short-term clinical outcomes. *J Cataract Refract Surg* 2011;37(3):441-445
- 15 Alió JL, Plaza-Puche AB, Piñero DP, Javaloy J, Ayala MJ. Comparative analysis of the clinical outcomes with 2 multifocal intraocular lens models with rotational asymmetry. *J Cataract Refract Surg* 2011;37(9):1605-1614
- 16 Olsen T. Calculation of intraocular lens power: a review. *Acta Ophthalmol Scand* 2007;85(5):472-485
- 17 Camps VJ, Piñero DP, de Fez D, Mateo V. Minimizing the IOL power error induced by keratometric power. *Optom Vis Sci* 2013;90(7):639-649
- 18 Camps VJ, Piñero DP, de Fez D, Coloma P, Caballero MT, Garcia C, Miret JJ. Algorithm for correcting the keratometric estimation error in normal eyes. *Optom Vis Sci* 2012;89(2):221-228
- 19 Retzlaff JA, Sanders DR, Kraff MC. Development of the SRK/T intraocular lens implant power calculation formula. *J Cataract Refract Surg* 1990;16(3):333-340
- 20 Haigis W. The Haigis formula. In Shammas HJ, ed. *Intraocular Lens Power Calculations*. Thorofare, NJ: Slack; 2004:41-57
- 21 Hoffer KJ. The Hoffer Q formula: a comparison of theoretic and regression formulas. *J Cataract Refract Surg* 1993;19(6):700-712
- 22 Holladay JT, Prager TC, Chandler TY, Musgrove KH, Lewis JW, Ruiz RS. A three-part system for refining intraocular lens power calculations. *J Cataract Refract Surg* 1988;14(1):17-24
- 23 Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;1(8476):307-310
- 24 Faria-Ribeiro M, Lopes-Ferreira D, López-Gil N, Jorge J, González-Méjome JM. Errors associated with IOL Master biometry as a function of internal ocular dimensions. *J Optom* 2014;7(2):75-78
- 25 Ho JD, Liou SW, Tsai RJ, Tsai CY. Estimation of the effective lens position using a rotating Scheimpflug camera. *J Cataract Refract Surg* 2008;34(12):2119-2127
- 26 Engren AL, Behndig A. Anterior chamber depth, intraocular lens position, and refractive outcomes after cataract surgery. *J Cataract Refract Surg* 2013;39(4):572-577
- 27 Norrby S. Sources of error in intraocular lens power calculation. *J Cataract Refract Surg* 2008;34(3):368-376
- 28 Preussner PR, Wahl J, Weitzel D, Berthold S, Kriechbaum K, Findl O. Predicting postoperative intraocular lens position and refraction. *J Cataract Refract Surg* 2004;30(10):2077-2083
- 29 Findl O, Drexler W, Menapace R, Georgopoulos M, Rainer G, Hitzenberg CK, Fercher AF. Changes in intraocular lens position after neodymium: YAG capsulotomy. *J Cataract Refract Surg* 1999;25:659-662
- 30 Piñero DP, Ayala Espinosa MJ, Alió JL. LASIK outcomes following multifocal and monofocal intraocular lens implantation. *J Refract Surg* 2010;26(8):569-577
- 31 Mohammadi SF, Rahman-A N, Mazouri A. Subjective refraction in eyes with multifocal IOLs. *J Refract Surg* 2011;27(3):16; author reply 162
- 32 van der Linden JW, Vrijman V, El-Saad R, van der Meulen IJ, Mourits MP, Lapid-Gortzak R. Autorefractive versus subjective refraction in a radially asymmetric multifocal intraocular lens. *Acta Ophthalmol* 2014;92(8):764-768